

Easy User Guide

CardioSoft 12 Lead ECG System


1

Connect the **CardioSoft ECG System** to your **PC** or **Laptop**.



7

The patient's **ECG** will then appear on screen.

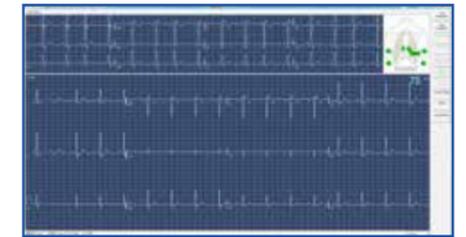

2


Open the patient's **clinical record** in your clinical system.



Note: INPS Hosted and AEROS sites must ensure that Numed Enterprise Link software is running on the remote desktop

8

Once you are happy with the ECG trace, press the **'ECG Acquisition'** button. There may be a delay of up to 10 seconds whilst the ECG is acquired.

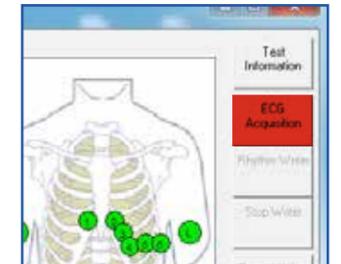


3

Double click the **I³** icon, this is usually found on your taskbar or desktop. This will **launch** the **I³** software.



9

Once the acquisition process has completed press **'Post Test Review'**.

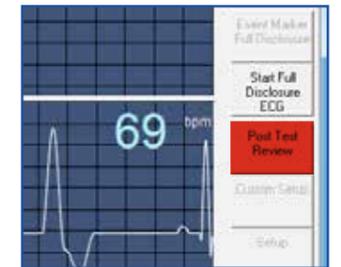

4

Click the **'Start'** button.



10

To begin the filing process, **close** the **CardioSoft** software by clicking the **red cross** in the top right hand corner.




5

Select **'ECG'** from the product selection screen - if you have more than one ECG system you may need to select **'GE CAM-USB'**.




11

A **confirmation message** will be displayed when the **ECG** has been successfully uploaded to the patient record - click **'OK'** to complete the process.

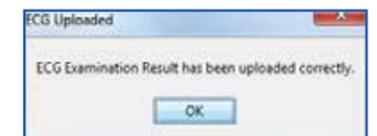

6

Confirm the patient's details are correct then click **'Yes'**.

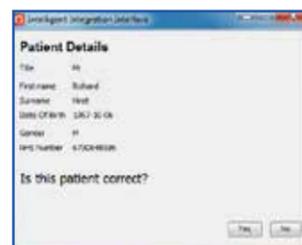

If you experience any problems using the **CardioSoft 12 Lead ECG System**, please contact our technical support team on: **0114 399 0010** or visit: **www.numed.co.uk/support**



SUPPLY | INSTALLATION | TRAINING | SUPPORT

Alliance House, Roman Ridge Road, Sheffield, S9 1GB Telephone: 0114 243 3896 Fax: 0114 243 3413



www.numed.co.uk



support@numed.co.uk